

# DOG IgE SPARCL™ ASSAY

## Life Diagnostics, Inc., Catalog Number: IGE-SP-4

### INTRODUCTION

IgE is the least abundant immunoglobulin in serum. It is involved in allergic reactions, binding to Fc receptors on basophils and mast cells. Subsequent binding of antigen to IgE triggers release of histamine and other vasoactive amines. IgE levels are elevated in asthma, eczema, rhinitis and parasitic infections. IgE is a potentially useful serum biomarker in such conditions.

### PRINCIPLE OF THE ASSAY

The dog IgE SPARCL™<sup>1</sup> (Spatial Proximity Analyte Reagent Capture Luminescence, ref 1) assay uses two dog IgE monoclonal antibodies developed at Life Diagnostics, Inc. Monoclonal IGE-4-13H5 is conjugated to horseradish peroxidase (HRP) and monoclonal IGE-4-4D1 is conjugated to acridan, a chemiluminescent substrate. When HRP and acridan conjugated antibodies bind to IgE they are brought into close proximity. With the addition of hydrogen peroxide, HRP catalyzes oxidation of proximal acridan molecules causing a flash of chemiluminescence. Acridan conjugated antibodies distant from HRP produce no signal. This principle allows the development of a homogeneous assay that allows rapid determination of IgE concentrations.

The HRP and acridan conjugated antibodies provided with the kit are mixed with standards and diluted samples in wells of the 96-well white SPARCL™ plate provided with the kit<sup>2</sup>. After incubation for 30 minutes on a shaker at 25°C and 150 rpm, the plate is placed into a luminometer. Trigger solution containing hydrogen peroxide is injected into each well and luminescence is immediately measured. The concentration of IgE is proportional to luminescence and is derived from a standard curve.

### MATERIALS AND COMPONENTS

#### Materials provided with the kit:

- Anti-IgE HRP stock **Store ≤ -70°C**
- Anti-IgE acridan stock **Store ≤ -70°C**
- IgE stock (lyophilized) **Store ≤ -70°C**
- Diluent; CSD50-1, 2 x 50 ml
- Trigger solution; TS7-1, 7 ml
- White SPARCL™ plate (12 x 8-well)
- Clear untreated 96-well plate

#### Materials required but not provided:

- Precision pipettes and tips
- Polypropylene microcentrifuge tubes
- Vortex mixer
- Plate incubator/shaker
- Luminometer capable of simultaneous injection/measurement
- Curve fitting software


### STORAGE

Store the HRP conjugate, acridan conjugate, and IgE stock at or below -70°C. The remainder of the kit should be stored at 2-8°C. The SPARCL™ plate should be kept in a sealed bag with desiccant and antioxidant. The kit will remain stable for at least six months from the

date of purchase, provided that the components are stored as described.

### GENERAL INSTRUCTIONS

1. Please take the time to completely read all instructions before starting your assay. Contact us if you need clarification.
2. All reagents used in the assay should be allowed to reach room temperature (25°C) before use.
3. It is important that standards and samples be added to the SPARCL™ plate quickly. If testing many samples, rather than pipetting standards and samples directly into the white SPARCL™ plate using a single channel pipettor, we recommend the following. First, pipette an excess volume of standards and samples into appropriate wells of the clear 96-well plate. Then use an 8- or 12-channel multipipettor to quickly and efficiently transfer 50 µl aliquots to the appropriate wells of the white SPARCL™ plate. The wells of the clear plate have a maximum volume of 300 µl.
4. Follow the sequence of events below when running the assay.

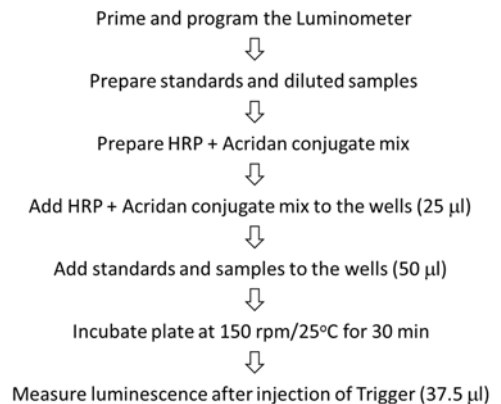

### STANDARD PREPARATION

1. Shortly before use thaw the dog IgE stock<sup>3</sup>.
2. Label 8 polypropylene tubes as 100, 50, 25, 12.5, 6.25, 3.13, 1.56 and 0.78 ng/ml.
3. Into the tube labeled 100 ng/ml, pipette the volume of diluent detailed on the stock vial label. Then add the indicated volume of stock and mix gently. This provides the 100 ng/ml standard.
4. Dispense 150 µl of diluent into the tubes labeled 50, 25, 12.5, 6.25, 3.13, 1.56 and 0.78 ng/ml.
5. Pipette 150 µl of the 100 ng/ml IgE standard into the tube labeled 50 ng/ml and mix. This provides the 50 ng/ml IgE standard.
6. Similarly prepare the remaining standards by two-fold serial dilution.

Store unused IgE stock at or below -70°C.

<sup>1</sup> The SPARCL™ technology was developed by Lumigen Corp.

<sup>2</sup> The white SPARCL™ plate provided with the kit has been treated with a reagent that reduces background chemiluminescence. Untreated plates cannot be used.

<sup>3</sup> IgE concentration of the stock was determined using purified dog IgE obtained from Bethyl Laboratories.

## SAMPLE PREPARATION

In studies at Life Diagnostics, we tested serum samples from 38 dogs identified as sick by veterinarians. IgE levels were  $18.0 \pm 35.3 \mu\text{g/ml}$  (mean $\pm$ SD), ranging from 0.1 to 192  $\mu\text{g/ml}$ . Because of the wide range of possible IgE concentrations, we suggest testing each sample at dilutions of both 100- and 2000-fold. We found that this approach gave at least one value within range of the standard curve. To avoid matrix effects do not test samples at dilutions less than 100-fold. Only use the diluent provided with the kit for dilution purposes.

## CONJUGATE MIX PREPARATION

Instructions for preparation of the conjugate mix are detailed on the box that contains the HRP and acridan conjugates. Prepare the mix shortly before use with diluent CSD50-1.

## LUMINOMETER SETUP

1. The luminometer must be capable of injection and simultaneous measurement of luminescence without any delay.
2. Prime the luminometer injection port with at least 1 ml of trigger solution.
3. Place the injection needle into the injection port, (necessary for BMG luminometers).
4. Program the luminometer to inject 37.5  $\mu\text{l}$  of trigger solution per well and to measure from time zero for 1 second (50 x 0.02 second intervals).
5. Define the format of the assay using the luminometer software.
6. Because the white SPARCL™ plate is provided as a 12 x 8-well strips, allowing use of fewer than 96-wells, make sure that the luminometer is programmed to inject trigger solution only into the wells being used.
7. We use a BMG LUMIstar Omega set at a gain of 3600. Optimal gain should be determined by the end user.
8. There are a number of manufacturers of luminometers that are equipped to run a SPARCL™ assay. Please contact Life Diagnostics or Lumigen ([www.lumigen.com](http://www.lumigen.com)) to discuss your luminometer.

## PROCEDURE

1. Before starting the assay ensure that the luminometer is primed with trigger solution and that the injection needle is positioned in the injection port.
2. Secure the desired number of SPARCL™ 8-well strips in the holder. Immediately seal unused strips in the resealable bag with desiccant and antioxidant. Store unused strips at 2-8°C.
3. Aliquot 25.0  $\mu\text{l}$  of conjugate mix into each well.
4. Dispense 50.0  $\mu\text{l}$  of standards and diluted samples into the wells (we recommend that standards and samples be tested in duplicate).
5. Incubate on an orbital micro-plate shaker at 150 rpm and 25°C for 30 minutes.
6. After the 30-minute incubation, place the plate in the luminometer and measure luminescence after injection of trigger solution (37.5  $\mu\text{l}$ ).
7. Remove the plate from the luminometer and discard the used strips. Keep the plate frame if future use is intended.

## CALCULATION OF RESULTS


1. Before calculating results, review the raw data. If artefacts (RLU spikes) are apparent immediately after injection of trigger solution, eliminate that portion of the luminescence profile from analysis for all wells. We routinely use the sum of RLU values from a 100-980 ms data collection window.

2. Determine the sum of RLU values within the data collection window for the standards and samples.
3. Using graphing software, construct a standard curve by plotting the sum of the RLU values for the standards versus the  $\log_{10}$  of the IgE concentration and fit to a sigmoidal, 4PL model.
4. Derive the corresponding concentration of IgE in the samples from the standard curve (remember to derive the concentration from the antilog).
5. Multiply the derived concentration by the dilution factor to determine the concentration of IgE in the original sample.
6. If the sum of the RLU values of diluted samples fall outside the standard curve, samples should be appropriately diluted and re-tested.

## TYPICAL STANDARD CURVE

A typical standard curve with sum of RLU values plotted on the Y-axis versus  $\log_{10}$  IgE concentrations on the X-axis is shown below. This curve is for illustration only and should not be used to calculate unknowns. A standard curve must be run with each experiment.

IgE (ng/ml)	RLU
100	141410
50	89454
25	48810
12.5	11367
6.25	4597
3.13	2487
1.56	1287
0.78	738

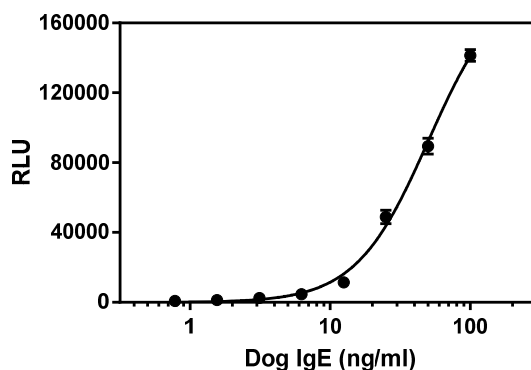

## REFERENCES

1. Akhavan-Tafti H. et al. A homogeneous chemiluminescent immunoassay method. *J Am Chem Soc.* 20;135(11):4191-4 (2013)

Rev 022218

For technical assistance please email us at [techsupport@lifediagnosics.com](mailto:techsupport@lifediagnosics.com)