

# HORSE SERUM AMYLOID A (SAA) SPARCL™ ASSAY

## Life Diagnostics, Inc., Catalog Number: SAA-SP-14

### INTRODUCTION

Serum amyloid A (SAA) is a positive acute phase protein of ~12 kDa that is expressed in the liver and circulates in blood. It is a useful biomarker of inflammation and disease in horses. Serum levels range from undetectable in normal horses to 1 mg/ml or greater in horses with colic (refs 1-3).

### PRINCIPLE OF THE ASSAY

The horse SAA SPARCL™<sup>1</sup> (Spatial Proximity Analyte Reagent Capture Luminescence, ref 4) assay uses two different peptide-specific horse SAA antibodies. One is conjugated to horseradish peroxidase (HRP), the other is conjugated to acridan, a chemiluminescent substrate. When the HRP and acridan conjugated antibodies bind to SAA they are brought into close proximity. With the addition of hydrogen peroxide, HRP catalyzes oxidation of proximal acridan molecules causing a flash of chemiluminescence. Acridan conjugated antibodies distant from HRP produce no signal. This principle allows the development of a homogeneous assay that allows rapid measurement of SAA concentrations.

Serum samples are first treated with reagent alcohol to dissociate SAA from lipoproteins. Diluted samples and standards are then mixed with the HRP and acridan-conjugated antibodies in the wells of the 96-well SPARCL™ plate<sup>2</sup> provided with the kit. After incubation for 30 minutes on a shaker at 25°C and 150 rpm, the plate is placed into a luminometer. Trigger solution containing hydrogen peroxide is injected into each well and luminescence is immediately measured. The concentration of SAA is proportional to luminescence and is derived from a standard curve.

### MATERIALS AND COMPONENTS

#### Materials provided with the kit:

- Anti-SAA HRP conjugate **Store ≤ -70°C**
- Anti-SAA acridan conjugate **Store ≤ -70°C**
- SAA stock **Store ≤ -70°C**
- Diluent; CSD50-1, 2 x 50 ml
- Trigger solution; TS7-1, 7 ml
- White SPARCL™ plate (12 x 8-well)
- Clear untreated 96-well plate

#### Materials required but not provided:

- Reagent alcohol<sup>3</sup>
- Precision pipettes and tips
- Polypropylene microcentrifuge tubes
- Vortex mixer
- Plate incubator/shaker
- Luminometer capable of simultaneous injection/measurement
- Curve fitting software


### STORAGE

Store the HRP conjugate, acridan conjugate and SAA stock at or below -70°C (they may be stored at -20°C for one week). The remainder of the kit should be stored at 2-8°C. The SPARCL™ plate should be kept in a sealed bag with desiccant and antioxidant. The

kit will remain stable for at least six months from the date of purchase, provided that the components are stored as described.

### GENERAL INSTRUCTIONS

1. Please take the time to completely read all instructions before starting your assay. Contact us if you need clarification.
2. All reagents used in the assay should be allowed to reach room temperature (25°C) before use.
3. It is important that standards and samples be added to the SPARCL™ plate quickly. If testing large numbers of samples, rather than pipetting standards and samples directly into the white SPARCL™ plate using a single channel pipettor, we recommend the following. First, pipette an excess volume of standards and samples into appropriate wells of the clear 96-well plate. Then use an 8- or 12-channel multipipettor to quickly and efficiently transfer 50 µl aliquots to the appropriate wells of the white SPARCL™ plate. The wells of the clear plate have a maximum volume of 300 µl.
4. Follow the sequence of events below when running the assay.

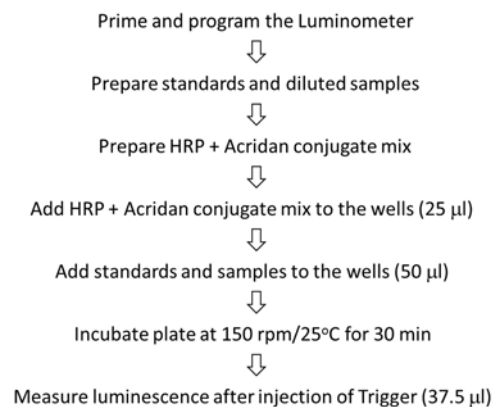

### STANDARD PREPARATION

The horse SAA stock is comprised of pure horse SAA diluted to 10 µg/ml in a glycerol containing carrier protein matrix.

1. Label five polypropylene tubes as 100, 50, 25, 12.5, and 6.25 ng/ml.
2. Into the tube labeled 100 ng/ml, mix 5 µl of the 10 µg/ml SAA stock with 495 µl of diluent. This provides the 100 ng/ml standard.
3. Dispense 150 µl of diluent into the tubes labeled 50, 25, 12.5, and 6.25 ng/ml.
4. Pipette 150 µl of the 100 ng/ml SAA standard into the tube labeled 50 ng/ml and mix. This provides the 50 ng/ml SAA standard.
5. Similarly prepare the remaining standards by two-fold serial dilution.

<sup>1</sup> The SPARCL technology was developed by Lumigen Corp.

<sup>2</sup> The plate provided with the kit has been treated with a reagent that reduces background chemiluminescence. Untreated plates cannot be used.

<sup>3</sup> Reagent Alcohol consists of ethanol, isopropyl alcohol and methanol in the ratio 90:5:5.

## SAMPLE PREPARATION

Prior to testing, serum samples must be treated with reagent alcohol to dissociate SAA from lipoproteins which interfere with SAA measurement. Rapidly mix 3 volumes of each serum sample (150.0 µl) with one volume (50.0 µl) of reagent alcohol. We recommend using either a positive displacement pipette or a Hamilton syringe to accurately dispense the reagent alcohol. Please note that after addition of alcohol the original sample is diluted 1.33 fold. The alcohol treated serum samples should be used within 15 minutes of preparation.

The alcohol treated samples must be further diluted at least 100-fold to avoid matrix effects. This can be achieved by mixing 2.50 µl of alcohol treated serum with 247.5 µl of diluent CSD50-1. Please note that this represents a 133.3-fold dilution of the original sample. If further dilution is needed, use CSD50-1. Do not use other diluents. Because the assay uses a homogeneous format it is susceptible to a prozone or "hook effect" at high SAA concentrations. Samples should ideally be tested at several dilutions in order to eliminate false low values.

## CONJUGATE MIX PREPARATION

Instructions for preparation of the conjugate mix are detailed on the box that contains the HRP and acridan conjugates. If necessary, after thawing, briefly centrifuge to ensure that the contents are at the bottom of the tubes. Prepare the mix shortly before use using the diluent provided with the kit.

## LUMINOMETER SETUP

1. The luminometer must be capable of injection and simultaneous measurement of luminescence without any delay.
2. Prime the luminometer injection port with 1 ml of trigger solution.
3. Place the injection needle into the injection port as needed for BMG luminometers.
4. Program the luminometer to inject 37.5 µl of trigger solution per well and to measure from time zero for 1 second (50 x 0.02 second intervals).
5. Define the format of the assay using the luminometer software.
6. Because the white SPARCL™ plate is provided as a 12 x 8-well strips, allowing use of fewer than 96-wells, make sure that the luminometer is programmed to inject trigger solution only into the wells being used.
7. We use a BMG LUMIstar Omega set at a gain of 3600. Optimal gain should be determined by the end user.
8. There are a number of manufacturers of luminometers that are equipped to run a SPARCL™ assay. Please contact Life Diagnostics or Lumigen ([www.lumigen.com](http://www.lumigen.com)) to discuss your luminometer.

## PROCEDURE

1. Before starting the assay ensure that the luminometer is primed with trigger solution and that the injection needle is positioned in the injection port.
2. Secure the desired number of SPARCL™ 8-well strips in the holder. Immediately seal unused strips in the resealable bag with desiccant and antioxidant. Store unused strips at 2-8°C.
3. Aliquot 25.0 µl of conjugate mix into each well.
4. Dispense 50.0 µl of standards and diluted samples into the wells (we recommend that standards and samples be tested in duplicate).
5. Incubate on an orbital micro-plate shaker at 150 rpm 25°C for 30 minutes.

6. After the 30-minute incubation, place the plate in the luminometer and measure luminescence after injection of trigger solution (37.5 µl).
7. Remove the plate from the luminometer and discard the used strips. Keep the plate frame if future use is intended.


## CALCULATION OF RESULTS

1. Before calculating results, review the raw data. If artefacts (RLU spikes) are apparent immediately after injection of trigger solution, eliminate that portion of the luminescence profile from analysis for all wells. We routinely use the sum of RLU values from a 100-980 ms data collection window.
2. Determine the sum of RLU values within the data collection window for the standards and samples.
3. Using curve fitting software, construct a standard curve by plotting the sum of RLU values of the standards versus SAA concentration in ng/ml. We find that a single site, total and nonspecific binding model works well.
4. Derive the concentration of SAA in the diluted samples from the standard curve.
5. Multiply the derived concentration by the dilution factor to determine the concentration of SAA in the serum or plasma sample.
6. If the sum of RLU values for the diluted samples fall outside the standard curve, samples should be diluted appropriately and re-tested.

## TYPICAL STANDARD CURVE

A typical standard curve is shown below. This curve is for illustration only. A standard curve must be run with each experiment.

SAA(ng/ml)	RLU
100	82900
50	62091
25	33348
12.5	8969
6.25	3192

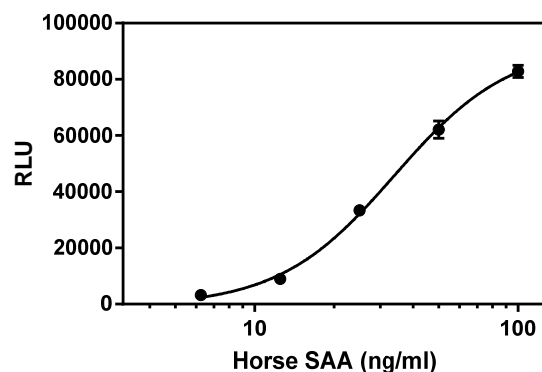

## REFERENCES

1. Jacobsen S and Andersen PH. The acute phase protein serum amyloid A (SAA) as a marker of inflammation in horses. *Equine vet. Educ.* 19:38-46 (2007)
2. Cywinska A. et. al. Serum amyloid A (SAA) concentration after training sessions in Arabian race and endurance horses. *BMC Veterinary Research* 9:91 (2013) <http://bmcvetres.biomedcentral.com/articles/10.1186/1746-6148-9-91>

3. Pihl TH. et. al. Influence of disease process and duration on acute phase proteins and peritoneal fluid of horses with colic. J Vet. Intern. Med. 29:651-658 (2015)
4. Akhavan-Tafti H. et al. A homogeneous chemiluminescent immunoassay method. J Am Chem Soc. 20;135(11):4191-4 (2013)

Rev 022118

For technical assistance please email us at  
[techsupport@lifediagnosics.com](mailto:techsupport@lifediagnosics.com)