

# MONKEY TRANSTHYRETIN SPARCL™ ASSAY

## Life Diagnostics, Inc., Catalog Number: TTR-SP-3

### INTRODUCTION

Transthyretin, also known as prealbumin, is a tetramer of a single ~14 kDa polypeptide. It is a serum transporter of thyroxine that complexes with retinol binding protein. In humans, it is used as a biomarker of nutritional status (ref 1) and has potential as a biomarker for Alzheimer's disease (ref 2). It is a negative acute phase reactant; the levels of which decrease during infection, inflammation and disease (ref 3). This kit allows measurement of transthyretin concentrations in serum or plasma from cynomolgus and rhesus monkeys.

### PRINCIPLE OF THE ASSAY

The monkey transthyretin SPARCL™<sup>1</sup> (Spatial Proximity Analyte Reagent Capture Luminescence, ref 4) assay uses two transthyretin specific antibodies. One is conjugated to horseradish peroxidase (HRP), the other is conjugated to acridan, a chemiluminescent substrate. When the HRP and acridan-conjugated antibodies bind to transthyretin they are brought into proximity. With the addition of hydrogen peroxide, HRP catalyzes oxidation of proximal acridan molecules causing a flash of chemiluminescence. Acridan conjugated antibodies distant from HRP produce no signal. This principle allows the development of a homogeneous assay that allows rapid measurement of transthyretin concentrations.

Diluted serum or plasma samples and standards are mixed with the HRP and acridan-conjugated antibodies in the wells of the 96-well SPARCL™ plate<sup>2</sup> provided with the kit. After incubation for 30 minutes on a shaker at 25°C and 150 rpm, the plate is placed into a luminometer. Trigger solution containing hydrogen peroxide is injected into each well and luminescence is immediately measured. The concentration of transthyretin is proportional to luminescence and is derived from a standard curve.

### MATERIALS AND COMPONENTS

#### Materials provided with the kit:

- Anti-transthyretin HRP conjugate. **Store ≤ -70°C**
- Anti-transthyretin acridan conjugate. **Store ≤ -70°C**
- Transthyretin stock. **Store ≤ -70°C**
- Diluent; CSD50-1, 2 x 50 ml
- Trigger solution; TS7-1, 7 ml
- White SPARCL™ plate (12 x 8-well)
- Clear untreated 96-well plate

#### Materials required but not provided:

- Precision pipettes and tips
- Polypropylene microcentrifuge tubes
- Vortex mixer
- Plate incubator/shaker
- Luminometer capable of simultaneous injection/measurement
- Curve fitting software


### STORAGE

Store the HRP conjugate, acridan conjugate and transthyretin stock at -70°C (they may be stored at -20°C for one week). The remainder of the kit should be stored at 2-8°C. The SPARCL™ plate should be kept in a sealed bag with desiccant and antioxidant. The kit will

remain stable for at least six months from the date of purchase, provided that the components are stored as described.

### GENERAL INSTRUCTIONS

1. Please take the time to completely read all instructions before starting your assay. Contact us if you need clarification.
2. All reagents used in the assay should be allowed to reach room temperature (25°C) before use.
3. It is important that standards and samples be added to the SPARCL™ plate quickly. If testing large numbers of samples, rather than pipetting standards and samples directly into the white SPARCL™ plate using a single channel pipettor, we recommend the following. First, pipette an excess volume of standards and samples into appropriate wells of the clear 96-well plate. Then use an 8- or 12-channel multipipettor to quickly and efficiently transfer 50 µl aliquots to the appropriate wells of the white SPARCL™ plate. The wells of the clear plate have a maximum volume of 300 µl.
4. Follow the sequence of events below when running the assay.

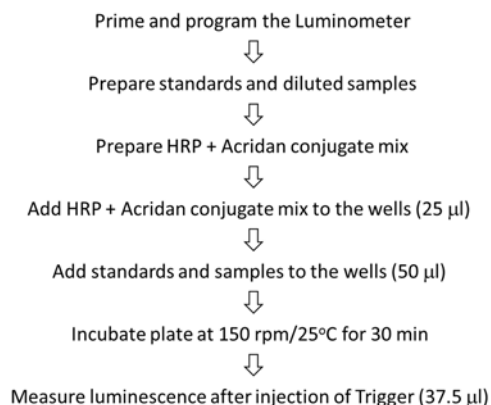

### STANDARD PREPARATION

Thaw the transthyretin stock shortly before use.

1. Label eight polypropylene tubes as 5, 2.5, 1.25, 0.625, 0.313, 0.156, 0.078 and 0.039 ng/ml.
2. Into the tube labeled 5 ng/ml, pipette the volume of diluent detailed on the stock vial label. Then add the indicated volume of transthyretin stock and mix gently. This provides the 5 ng/ml standard.
3. Dispense 150 µl of diluent into the tubes labeled 2.5, 1.25, 0.625, 0.313, 0.156, 0.078 and 0.039 ng/ml.
4. Pipette 150 µl of the 5 ng/ml transthyretin standard into the tube labeled 2.5 ng/ml and mix. This provides the 2.5 ng/ml transthyretin standard.
5. Similarly prepare the remaining standards by serial dilution. Use the standards within one hour of preparation.

### SAMPLE PREPARATION

In studies at Life Diagnostics, we found levels of 139.7±10.5 µg/ml (mean±SD, n=3) in serum from healthy monkeys. Levels in serum

<sup>1</sup> The SPARCL technology was developed by Lumigen Corp.

<sup>2</sup> The plate provided with the kit has been treated with a reagent that reduces background chemiluminescence. Untreated plates cannot be used.

from sick monkeys were  $43.9 \pm 21 \mu\text{g/ml}$  (mean  $\pm$  SD, n=6). We found it necessary to dilute serum 40,000-fold to obtain values within range of the standard curve. Optimal dilutions should, however, be determined by the end user.

A 40,000-fold dilution can be achieved as follows:

1. For each sample to be tested, dispense 247.5  $\mu\text{l}$  and 798  $\mu\text{l}$  of diluent into microcentrifuge tubes.
2. Pipette 2.5  $\mu\text{l}$  of serum or plasma into the tube containing 247.5  $\mu\text{l}$  of diluent and mix to give a 100-fold dilution.
3. Pipette 2.0  $\mu\text{l}$  of the 100-fold diluted sample into the tube containing 798  $\mu\text{l}$  of diluent and mix to give a 40,000-fold dilution.

### CONJUGATE MIX PREPARATION

Instructions for preparation of the conjugate mix are detailed on the box that contains the HRP and acridan conjugates. If necessary, after thawing, briefly centrifuge to ensure that the contents are at the bottom of the tubes. Prepare the mix shortly before use using the diluent provided with the kit.

### LUMINOMETER SETUP

1. The luminometer must be capable of injection and simultaneous measurement of luminescence without any delay.
2. Prime the luminometer injection port with 1 ml of trigger solution.
3. Place the injection needle into the injection port as needed for BMG luminometers.
4. Program the luminometer to inject 37.5  $\mu\text{l}$  of trigger solution per well and to measure from time zero for 1 second (50 x 0.02 second intervals).
5. Define the format of the assay using the luminometer software.
6. Because the white SPARCL™ plate is provided as a 12 x 8-well strips, allowing use of fewer than 96-wells, make sure that the luminometer is programmed to inject trigger solution only into the wells being used.
7. We use a BMG LUMIstar Omega set at a gain of 3600. Optimal gain should be determined by the end user.
8. There are a number of manufacturers of luminometers that are equipped to run a SPARCL™ assay. Please contact Life Diagnostics or Lumigen ([www.lumigen.com](http://www.lumigen.com)) to discuss your luminometer.

### PROCEDURE

1. Before starting the assay ensure that the luminometer is primed with trigger solution and that the injection needle is positioned in the injection port.
2. Secure the desired number of SPARCL™ 8-well strips in the holder. Immediately seal unused strips in the resealable bag with desiccant and antioxidant. Store unused strips at 2-8°C.
3. Aliquot 25.0  $\mu\text{l}$  of conjugate mix into each well.
4. Dispense 50.0  $\mu\text{l}$  of standards and diluted samples into the wells (we recommend that standards and samples be tested in duplicate).
5. Incubate on an orbital micro-plate shaker at 150 rpm 25°C for 30 minutes.
6. After the 30-minute incubation, place the plate in the luminometer and measure luminescence after injection of trigger solution (37.5  $\mu\text{l}$ ).
7. Remove the plate from the luminometer and discard the used strips. Keep the plate frame if future use is intended.


### CALCULATION OF RESULTS

1. Before calculating results, review the raw data. If artefacts (RLU spikes) are apparent immediately after injection of trigger solution, eliminate that portion of the luminescence profile from analysis for all wells. We routinely use the sum of RLU values from a 100-980 ms data collection window.
2. Determine the sum of RLU values within the data collection window for the standards and samples.
3. Using graphing software, construct a standard curve by plotting the sum of the RLU values for the standards versus the  $\log_{10}$  of transthyretin concentration and fit to a sigmoidal, 4PL model.
4. Derive the corresponding concentration of transthyretin in the samples from the standard curve (remember to derive the concentration from the antilog).
5. Multiply the derived concentration by the dilution factor to determine the concentration of transthyretin in the original sample.
6. If the sum of the RLU values of diluted samples fall outside the standard curve, samples should be appropriately diluted and re-tested.

### TYPICAL STANDARD CURVE

A typical standard curve is shown below. This curve is for illustration only and should not be used to calculate unknowns. A standard curve should be run with each experiment.

Transthyretin (ng/ml)	RLU
5.0	34881
2.5	18593
1.25	8522
0.625	3903
0.313	2182
0.156	1531
0.078	1067
0.039	1102

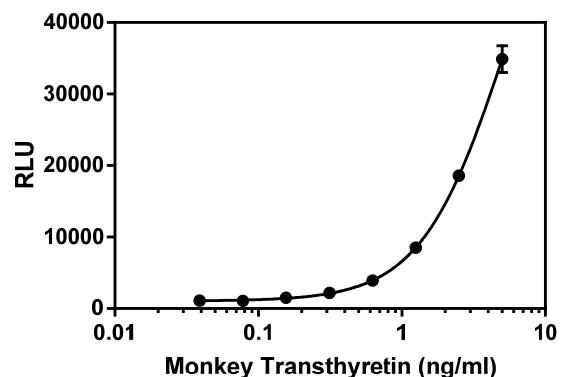

### REFERENCES

1. Bharadwaj S. et al. Malnutrition: laboratory markers vs nutritional assessment. *Gastroenterology Report* 4(4):272-280 (2016)
2. Velayudhan L. et al. Plasma transthyretin as a candidate marker for Alzheimer's disease. *Journal of Alzheimer's Disease*. 28:369-375 (2012)
3. Banks RE. et al. The acute phase response in patients receiving subcutaneous IL-6. *Clin Expo Immunol*. 102:217-223 (1995)

4. Akhavan-Tafti H. et al. A homogeneous chemiluminescent immunoassay method. *J Am Chem Soc.* 20;135(11):4191-4 (2013)

Rev 022118

For technical assistance please email us at  
[techsupport@lifediagnostics.com](mailto:techsupport@lifediagnostics.com)